



Voltammetric determination of copper in seawater at a glassy carbon disk electrode modified with Au@MnO₂ core-shell microspheres

Hong Wei¹ · Dawei Pan^{2,3} · Xueping Hu² · Ming Liu¹ · Haitao Han² · Dazhong Shen¹

Received: 29 January 2018 / Accepted: 12 April 2018
© Springer-Verlag GmbH Austria, part of Springer Nature 2018

Abstract

Anodic stripping voltammetric determination of copper ions was accomplished at a glassy carbon disk electrode modified with core-shell microspheres of the gold@manganese dioxide (Au@MnO₂) type. These were synthesized via electrochemical deposition. The gold nanoparticles (AuNPs) were electrochemically deposited and employed as an active support material for the growth of MnO₂ to yield Au@MnO₂ core-shell particles with unique and regular spherical morphology. The microspheres have a diameter of 200–250 nm and scrolled edges like a cactus. Due to the absorption capacity of MnO₂ and the electrocatalytic ability of the AuNPs, an excellent anodic signal is obtained for copper ions. Response is linear in the 20 nM to 1 μM copper ion concentration range, with a 4.9 ± 0.2 nM ($n = 3$) detection limit under optimized conditions. The electrode is stable and excellently reproducible. It was successfully applied to the analysis of copper ions in spiked seawater samples.

Keywords Core-shell microspheres · Manganese dioxide · Cyclic voltammetry · Differential pulse voltammetry · Electrochemical deposition · Adsorption · Scanning electron microscopy

Introduction

Copper, an indispensable trace element in human beings, plays a significant role in normal physiological conditions since it is

not only an essential component of several enzymes but also involved in the transport of Fe [1, 2]. Copper, a great hazard of metal pollutants, has a severe toxicity as a result of its extensive use and complex distribution in the environment. Especially in the ocean environment, copper ions directly exposed to marine organisms can cause bio-accumulation and endanger people's health eventually. As we know, the aquo-complexed “free” cupric ion (Cu²⁺) rather than the inorganic or organic complexes [3] cause greatly harm to the environment. Thus, it is important to have a reliable and sensitive analytical method for accurately detecting copper ions in the ocean environment. Many methods have been investigated to detect copper ions, such as UV–vis spectrometer or visual (bare-eye) determination [4], flame atomic absorption spectrometry (FAAS) [5], inductively coupled plasma spectrometry (ICP-MS) [6, 7], and X-ray fluorescence spectrophotometry (XRFS) [8]. However, these methods are relatively time-consuming, fiddly and costly. Comparatively, the properties of short analysis time, low power consumption, and inexpensive equipment without any prior separation, inherent miniaturization and portability [9–11] make stripping voltammetry prominent in the field of electrochemical analytical chemistry.

Gold possesses unique properties, such as fast electron transfer rate, excellent bio-compatibility and high catalytic

Electronic supplementary material The online version of this article (<https://doi.org/10.1007/s00604-018-2799-1>) contains supplementary material, which is available to authorized users.

✉ Dawei Pan
dwpan@yic.ac.cn

✉ Dazhong Shen
dzshen@sdnu.edu.cn

¹ College of Chemistry, Chemical Engineering and Materials Science, Collaborative Innovation Center of Functionalized Probes for Chemical Imaging in Universities of Shandong, Key Laboratory of Molecular and Nano Probes, Ministry of Education, Shandong Provincial Key Laboratory of Clean Production of Fine Chemicals, Shandong Normal University, Jinan 250014, People's Republic of China

² Key Laboratory of Coastal Environmental Processes and Ecological Remediation, Yantai Institute of Coastal Zone Research, Chinese Academy of Sciences, Yantai 264003, People's Republic of China

³ University of Chinese Academy of Sciences, Beijing 100049, People's Republic of China

activity [12–14]. In addition, some researchers had found that the performance of the electrode could be improved by the deposition of metal particles. For example, Ashis Das et al. [15] used the electrodeposition of tin nanorods on glassy carbon electrodes and selectively detected progesterone using voltammetric method. In Wang groups [16], a well-defined three-dimensional gold hierarchical dendrites was prepared by one-step electrodeposition on a glassy carbon electrode and had amplification detection of Pb^{2+} with high sensitivity. Lu et al. [13] used a screen-printed carbon electrode (SPCE) co-modified with an in-situ plated bismuth (Bi) particles for determination of the Zn(II), Pb(II) and Cu(II) ions. As we know, the adsorption can improve the selectivity and sensitivity of the modified electrode. For many years, metal oxide had attracted wide attention in the aspect of detection and removal of heavy metals [16–18], where manganese dioxide was particularly prominent in terms of excellent adsorption ability [18–20]. Moreover, manganese dioxide is considered to be an economical and easy accessible adsorbent in the environment. Some researchers were synthesized several times for Au-MnO₂ nanomaterials before. Veeramani et al. [21] did synthesize of an Au-MnO₂ nanocomposite dispersed on an electrophoretically prepared graphene surface. Qiu groups [22] synthesized Au@MnO₂ core-shell nanomesh structure on a flexible polymeric substrate through nanosphere lithography combined with electro-deposition processing.

As reported, various modified electrodes had been employed to measure copper ions, such as rGO-AuNPs modified GCE [23], AuNP-SPCE electrode [24], NH₂-rGO/ β -CD electrode [25], PPyNWs^g electrode [12], Bi-AuNPs/SPE electrode [13], etc. The above practical electroanalysis were performed in tap waters, lake waters or waster waters. When the real seawater samples were concerned, the salinity is a big problem. Although determination of copper ions in seawater was reported previously in our group [14], the direct analysis of free copper ions in seawater was still a challenge. Thus, the effect of different salinity of seawater on the application of our electrode was also be tested in this paper.

In this study, more effectively operations to synthesize Au@MnO₂ core-shell structure, just through electrodeposition processing, were taken. Au nanoparticles were employed as active support materials and which can speed up the rate of MnO₂ crystal production. Eventually, a novel type core-shell microspheres Au@MnO₂ was formed by electrochemical deposition. Core-shell microspheres Au@MnO₂ composites were used for copper ions determination in consideration of the electrocatalytic properties of gold and the excellent absorption capacity of MnO₂. The Au@MnO₂ modified electrode showed remarkable sensitivity and selectivity in voltammetric measurement of copper ions with a lower detection limit. In addition, this novel core-shell microsphere Au@MnO₂ modified electrode also applied for the determination of copper ions in seawater.

Experimental

Chemicals and solutions

Standard stock solution of copper was purchased from Acros Organics(USA. <http://www.acros.com/>). Chlorauric acid (HAuCl₄) was supplied by Sinopharm Chemical Reagent (Shanghai, China. <http://www.sinoreagent.com.cn/>). Manganese(II) acetate tetrahydrate (MnAc₂·4H₂O) was purchased from Sinopharm Chemical Reagent (Shanghai, China. <http://www.sinoreagent.com.cn/>). All other chemicals were analytical reagents that have not been further purified. Standard artificial seawater (salinity of 29.998 and 4.998) were purchased from Beijing Putian Tongchuang Biological Technology Co. (Beijing, China. Ltd. <http://www.gbwl14.com/>). Deionized water (18.2 M Ω cm specific resistance), obtained from Pall Cascada laboratory water system (USA. <http://www.pall.com/main/home.page>), was used throughout the experience.

Apparatus

The morphology of Au, MnO₂, Au@MnO₂ modified electrodes were recorded on scanning electron microscopy and Back Scattered Electron (BSE) Imaging (SEM Hitachi S-4800 microscope, Japan. <http://www.hitachi.com/>), energy dispersive X-ray spectroscopy (EDX HORIBAEX-350 Japan. <http://www.horiba.com/>), X-ray diffraction spectroscopy (XRD ADVANCE-D8 Germany. <https://www.bruker.com/cn.html>) and X-ray photoelectron spectroscopy (XPS Escalab-250 USA. <https://www.thermofisher.com>). The comparative testing were used ICP-MS (ELAN DRC, Perkin Elmer Instruments, USA. <http://www.perkinelmer.com/>). All electrochemical experiments were performed with an Electrochemical Work Station (CHI 660E, CH Instruments, Inc. Shanghai, China. <http://chi.instrument.com.cn/>) carried out in a conventional three-electrode cell. A modified glassy carbon (GC) disk (3 mm in diameter, Chenhua Instruments, Shanghai, China. <http://chi.instrument.com.cn/>) was used as the working electrode, with Ag/AgCl and platinum foil serving as the reference and counter electrodes, respectively.

Preparation of Au@MnO₂ microsphere modified electrode

Prior to modification, the GC electrode was thoroughly polished with 0.3 μm and 0.05 μm aqueous slurries of alumina powder, and then sonicated for 3 min in ethanol and water respectively. Core-shell Au@MnO₂ microspheres were synthesized via two-step electrochemical deposition. Firstly, the GC electrode was immersed in 1.0 mM chlorauric acid containing 0.2 M sodium sulfate solution to electrochemically electrodeposit Au nanoparticles with constant potential at -0.2 V for

15 s. Then the gold modified electrode was rinsed with ultrapure water thoroughly. Then manganese oxide were deposited on Au modified electrode by cycling the deposition potential (scan rate of 0.2 V s^{-1}). The electrode was cycling from 0.0 V to 0.9 V in 1 mM manganese(II) acetate tetrahydrate and 1 mM sodium sulfate for 8 cycles. Then the obtained GC/Au@MnO₂ was washed carefully with deionized water and then dried at room temperature. Scheme 1 illustrated the stepwise assembly process of the Au@MnO₂ modified electrode. For comparison, Au or MnO₂ coated GCE was prepared with the same process, respectively.

Electrochemical analysis procedure

Unless stated otherwise, the experiments were carried out in the 0.1 M acetate buffer (pH 5.0). Differential pulse voltammetry (DPV) scans over the potential range from 0 V to 0.6 V were recorded by using the following parameters: amplitude of 0.05 V, pulse width of 0.2 s, pulse period of 0.5 s, and an equilibrium time of 2 s. Prior to the next cycle, the electrode was cleaned for 30 s at 0.6 V with stirring.

Preparation of real samples

Seawater sample was collected from the local (Yellow Sea, Shandong Province, China). The sample treatment was prepared as follows: all the seawater samples were filtered ($0.45 \mu\text{m}$ membrane filters) in acid-cleaned polyethylene bottles and kept at 4°C until determination. The sample seawater was acidified with a certain amount of HNO₃ and H₂O₂ was added to adjust the pH of water samples less than 2.0, finally digested samples in quartz tubes using a 500 W UV lamp (Metrohm MVA-UV 705, Switzerland). Standard artificial seawater did not need any treatment, and was directly applied to the detection of copper ions.

Results and discussion



Choice of materials

Various materials had been used to preparation of modified electrodes for improvement of the selectivity and sensitivity in copper determination, such as PPy [12], PANI [26], rGO [23],


GQDs [27], AgNPs [28], ZnO [29], SiO₂ [30], etc. In contrast, AuNPs had unique excellent catalytic performance better than AgNPs, which had been widely studied for practical applications in many fields such as catalysis, nanodevices, and electroanalysis [12, 13]. Manganese dioxide was particularly prominent in terms of excellent adsorption ability [18–20]. It was also considered as an economical and accessible adsorbent in the environment instead of PPy and PANI. In particular, the excellent intrinsic conductivity of AuNPs could speed up the growth rate of MnO₂, resulting in the form of core-shell microspheres Au@MnO₂.

Morphology of Au@MnO₂ microsphere modified electrode

The SEM micrographs of Au nanoparticles, MnO₂ and Au@MnO₂ were shown in Fig. 1. BSE micrograph, EDX, XRD and XPS images were also used to characterize the composites. The respective data and explanations were given in the Electronic Supporting Material (ESM). In Fig. 1a, the spherical Au is compactly coated on the GCE surface with size distribution ranging from 50 nm to 100 nm. As shown in Fig. 1b, the morphology of flaky MnO₂ are rough, non-uniform and crowded together with scrolled edges form. Figure 1c, d show the surface morphology of the Au@MnO₂ modified electrode at different magnifications. The Au@MnO₂ surface morphology is spherical with largely scrolled edges form. The shape of Au@MnO₂ was uniform and the size distribution ranged from 200 nm to 250 nm. The core-shell structure morphology formation mechanism is described in detail in the following part. The Au@MnO₂ composite possesses a core-shell structure, in which Au nanoparticles are employed as active support material and the fate of the Mn³⁺ intermediate is a key feature of this electrodeposition mechanism. In Eq. 1, the MnO₂ are formed from Mn²⁺ via electrochemical oxidation, and this process can be explained as a three-step model (Eq. 2–4) suggested by Paul and Cartwright [31]:



Scheme 1 The schematic illustration of the stepwise assembly procedure

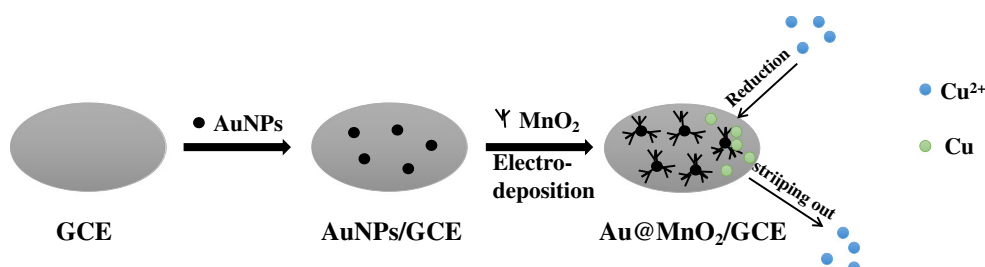

The formation of MnO_2 depends on the substrate [32]. Gold nanoparticles were used in here. Since Au nanoparticles might promote the rapid growth of Mn^{3+} , the morphology of MnO_2 would be changed. Growth began as the thin film along gold grain boundaries, soluble Mn^{3+} are produced initially, followed by MnOOH . The initial morphology is determined by the stability of soluble Mn^{3+} species. The growth of MnO_2 occurs primarily through the precipitation of a 2D film of MnOOH , which rapidly covers the surface of gold nanoparticles in all directions. Eventually, the entire surface of the sample is covered with core-shell Au@MnO_2 microspheres.

Electrochemical behavior of Au@MnO_2 microsphere modified electrode

The electrochemical behavior of the GC/Au@MnO_2 electrode at different buffers are investigated. As shown in Fig. S4, the redox peaks are significantly differentiated with the various buffer. The electrochemical oxidation and reduction of Au@MnO_2 disappeared when the pH value of the acetate buffer is larger than 5.0. In addition, taking into account the stable existence of copper ions, 0.1 M acetate buffer of pH 5.0 is chosen for the experiment.

The cycle voltammetry behavior of various electrodes were studied in 0.1 M acetate buffer (pH 5.0). The potential range was from -0.2 V to 1.3 V. As is shown in Fig. 2, the bare GCE (curve a) has no obvious redox peaks in the CV within the scan range. Besides, CV of the Au modified electrode (curve b) showed two obvious redox peaks in the potential

ranges of 0.6 – 0.7 V, 1.0 – 1.1 V. In curve c, the CV of the MnO_2 modified electrode also shows two apparent redox peaks in the potential ranges of 0.5 – 0.6 V, 0.75 – 0.85 V. Moreover, the current of Au@MnO_2 composite modified electrode (curve d) has redox peaks of both the Au modified electrode and the MnO_2 modified electrode. These results showed that MnO_2 and Au is effectively stable on the electrode surface, and these electrochemical results further demonstrated that it is quite effective that the core-shell microspheres of Au@MnO_2 combined to the electrode surface.

Electrochemical impedance spectrum (EIS) was used to verify the capability of electron transfer of copper ions at different electrodes. The semicircle diameter of EIS, equal to the electron transfer resistance (R_{et}), was depended on the dielectric features at the electrode and electrolyte interface. As shown in Fig. 3, the Nyquist diagrams of bare GC (a), GC/MnO_2 (b), GC/Au (c) and GC/Au@MnO_2 (d) were measured in 5 mM $\text{Fe(CN)}_6^{3-/4-}$ solution containing 0.5 M KCl. A semicircle of about $37\ \Omega$ in diameter for bare (curve a), after modified by MnO_2 (curve b), the semicircle diameter was remarkably increased to about $110\ \Omega$ in diameter. It was clearly observed that R_{et} of MnO_2 modified electrode (curve b) was significantly larger than that of bare GC (curve a). A semicircle for Au@MnO_2 (curve d) modified electrode was about $20\ \Omega$ in diameter, while the semicircle for Au (curve c) modified electrode was about $13\ \Omega$ in diameter. The R_{et} of Au@MnO_2 modified electrode was significantly reduced compared with R_{et} of MnO_2 modified electrode. The phenomenon was due to the excellent electronic transfer ability of

Fig. 1 SEM image of the GC/Au (a), GC/MnO_2 (b) and GC/Au@MnO_2 (c and d)


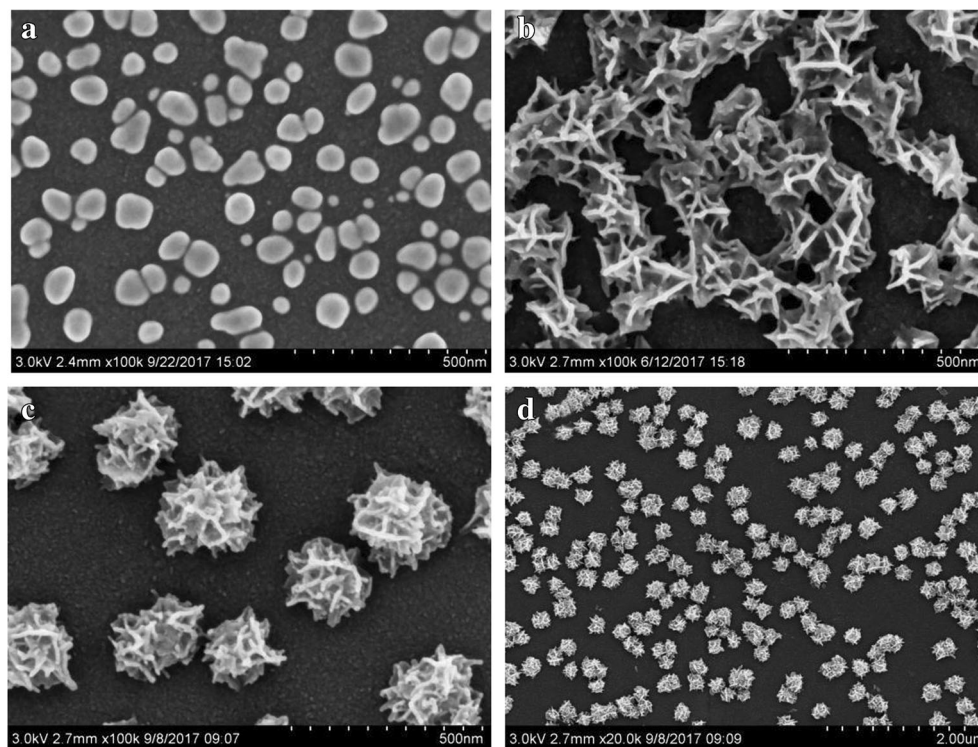


Fig. 2 CVs of bare GCE (a), GC/Au (b), GC/MnO₂ (c) and GC/Au@MnO₂ (d) in 0.1 M acetate buffer (pH 5.0) in the potential range of 0.2 to 1.3 V. Scan rate: 100 mV s⁻¹

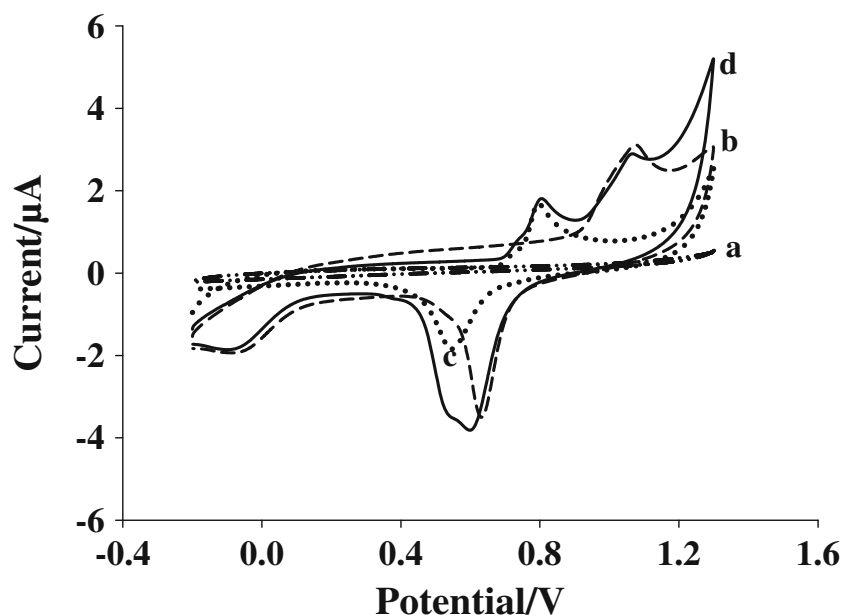

AuNPs which promotes the $[\text{Fe}(\text{CN})_6]^{3-}/[\text{Fe}(\text{CN})_6]^{4-}$ redox process. These results indicated that the electron transfer of copper ions at the Au@MnO₂ modified electrode was a typical electron transfer-limited process.

As shown in Fig. 4, the redox behaviors of copper ions at the modified electrode are studied by DPASV. No anodic signal of copper ions is seen on the bare GCE (Fig. 4a). The DPASV response for Au@MnO₂ coated GCE (Fig. 4d) is greatly larger than the response for MnO₂ coated GCE (Fig. 4b) and Au coated GCE (Fig. 4c), which can be seen in Fig. 4. More importantly, the responses current at the core-shell Au@MnO₂ modified electrode is larger than the sum of the

currents at the MnO₂ and Au nanoparticles single modified electrodes, indicating that MnO₂ combined with Au nanoparticles synergistically improves the anodic current response of copper ions. These results indicate that the response current of copper ions can be obviously increased by electrocatalytic synergistic and adsorption.

Mechanism of copper ions determination

In the anode stripping analysis, the target is very important for the effective adsorption of the surface on the modified electrode. It was clearly illustrated that the electrochemical

Fig. 3 Nyquist plots of bare GCE (a), GC/MnO₂ (b), GC/Au (c) and GC/Au@MnO₂ (d) in 5 mM $\text{Fe}(\text{CN})_6^{3-/4-}$ and 0.5 M KCl solutions


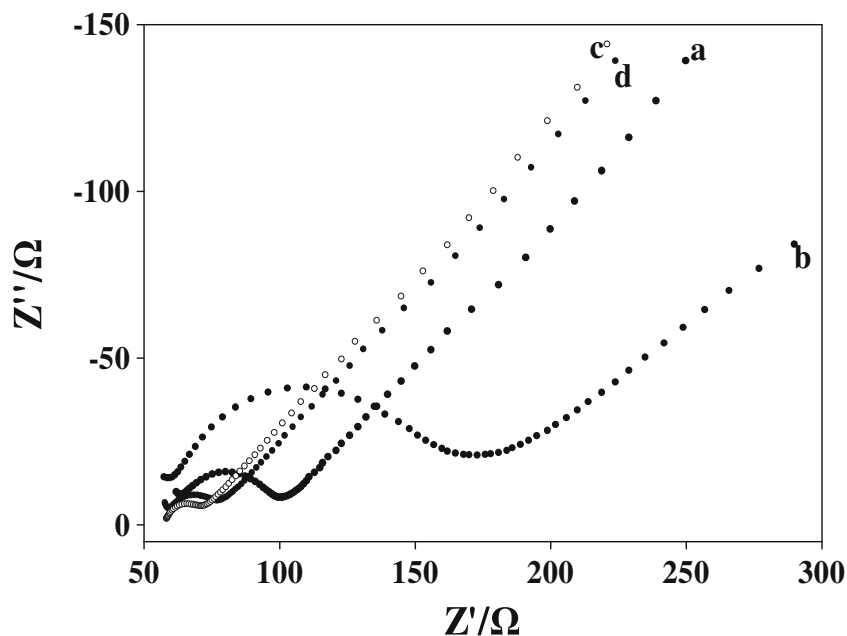


Fig. 4 DPASV of bare GCE (a), GC/Au (b), GC/MnO₂ (c), GC/Au@MnO₂ (d) in 0.1 M acetate buffer (pH 5.0) containing 200 nM copper ions. Scan rate: 50 mV s⁻¹

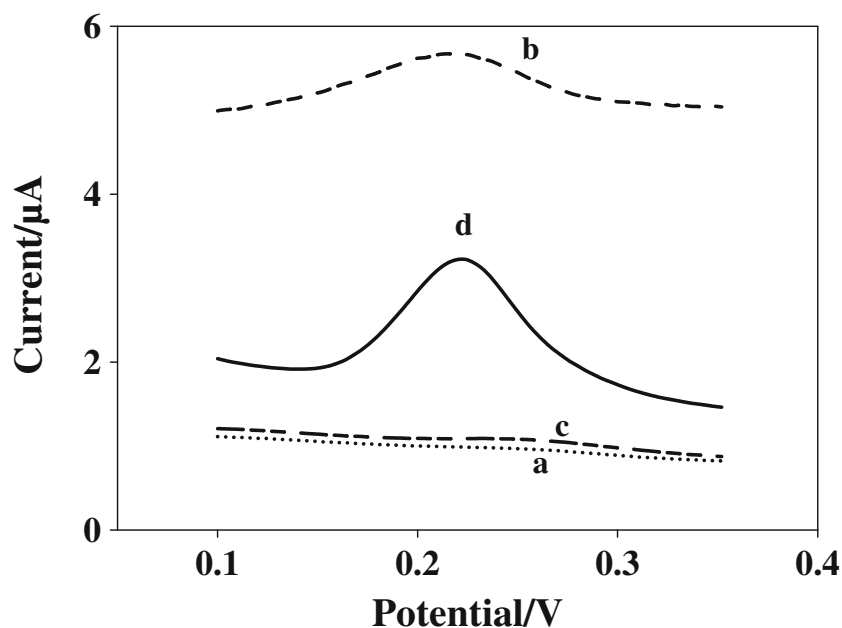

detection interfaces were based on Au nanoparticles as a coupling medium, and the Au nanoparticles were used for the bridging of MnO₂ and the glassy carbon electrode to transfer electrons.

At this stage, the large amounts of copper ions were accumulated on the surfaces of the MnO₂ via adsorption. Then the electrons transfer to the surface of the Au or glassy carbon electrode. When the potential is kept in the scope of deposition region, copper ions can be reduced on the surface of the MnO₂. However, the copper ions in the lower part of the aqueous solution can not be reduced. In this way, copper ions were adsorbed on the surface of the flaky MnO₂ and then

stripped out. And also, the more copper ions were adsorbed on the surface of core-shell composites, the more it would be reduced, accordingly, the stripping peak response was enhanced. This demonstrated that the modified electrode possessed good electrochemical response to copper ions.

Optimization for copper ions measurement on Au@MnO₂ microsphere modified electrode

The following parameters were optimized: (a) deposition potential; (b) deposition time; (c) pH value of the buffer; Respective data and Figures were given in the ESM. The

Fig. 5 The calibration plot for copper ions ($n = 3$). Left: DPASV of the GC/Au@MnO₂ at different copper ions concentrations (from 0.02 μM to 1 μM) in 0.1 M acetate buffer (pH 5.0). Scan rate: 50 mV s⁻¹

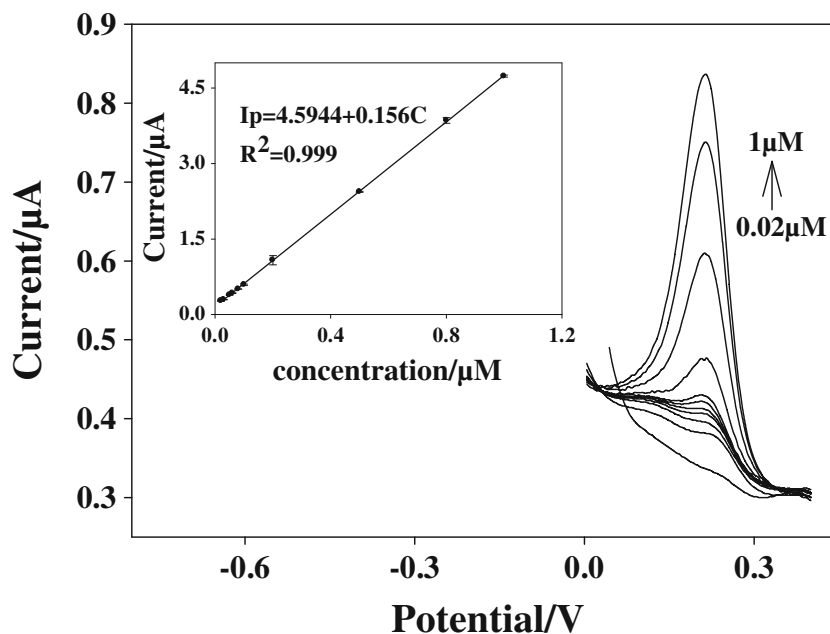


Table 1 Comparison of the analytical performance and other analytical methods for copper ions determination

| Methods | Electrode/agents | Linear range (μM) | Detecting limit (μM) | Applicable waters | References |
|-------------------|--|--------------------------------|-----------------------------------|-------------------|--------------|
| Colorimetric | Br-PEI-AuNPs ^a | 0.1–10 | 0.03 | Lake waters | [4] |
| FAAS | Alumina-SDS ^b | No | 0.04 | Tap waters | [5] |
| ICP-MS | Ascorbic acid | 0.008–0.8 | 0.01 | Seawaters | [7] |
| XRFS | No | 0.8–23 | 0.2 | Ascorbic acid | [8] |
| ECL ^c | Lucigenin | 0.03–1 | 0.002 | Tap waters | [11] |
| SWASV | rGO-AuNPs ^d | 1–12 | 0.03 | Tap waters | [23] |
| SWASV | AuNP-SPCE | 0.02–2 | 0.00002 | Tap waters | [24] |
| SWASV | NH ₂ -rGO/ β -CD ^e | 0.03–100 | 0.003 | Lake waters | [25] |
| DNPV ^f | PPyNWs ^g | 0.05–1 | 0.05 | Waste waters | [12] |
| DPV | Bi-AuNPs/SPE | 0.02–2 | 0.0005 | Lake waters | [13] |
| DPV | Au@MnO ₂ | 0.02–1 | 0.005 | Seawaters | Present work |

^a Branched polyethylenimine functionalized gold nanoparticles

^b Nanometer-sized γ -alumina nanoparticles modified with sodium dodecyl sulfate (SDS)

^c Electrochemiluminescence

^d Reduced graphene oxide-gold nanoparticles

^e Amino-reduced graphene oxide and β -cyclodextrin

^f Differential normal pulse voltammetry

^g Polypyrrole nanowires

following experimental conditions were found to give best results: (a) deposition potential of -0.3 V ; (b) 60s deposition time; (c) the buffer (pH 5.0).

Calibration plot

To further evaluate the stripping performance of the paper method with DPASV, it was performed at the GC/Au@MnO₂ in 0.1 M acetate buffer (pH 5.0) under the optimal conditions. As is revealed in Fig. 5, the stripping voltammograms are corresponding with different concentrations of copper ions. The peak current increased linearly in the copper ions concentration ranging from 0.02 to 1 μM . The linear regression equation was expressed as follows:

$$I_p = 0.156C + 4.5944 \quad (0.02\text{--}1 \mu\text{M}, R^2 = 0.999)$$

The detection limit ($3\sigma/m$) with standard deviation for copper ions determination at the GC/Au@MnO₂ was $4.9 \pm 0.2\text{ nM}$ ($n = 3$). Furthermore, comparison about copper ions determination by electrochemical and other analytical methods is shown in Table 1. Compared with other electrodes, the Au@MnO₂ modified electrode revealed higher efficiency, higher sensitivity, lower detection limit and wider linear range. The results indicates that the modified electrode may be a good choice for determination of copper ions.

Reproducibility, repeatability and interference

The reproducibility of Au@MnO₂ modified GCE, in the solution with 100 nM copper ions, was evaluated by six independently modified electrodes with the same method and the relative standard deviation (RSD) was 5.3%, respectively,

Table 2 Results of real seawater samples detected by Au@MnO₂ microsphere modified electrode and inductively coupled plasma mass spectrometry (ICP-MS) methods

| Real samples | Copper ions added (nM) | Mean (nM) \pm SD | | Recovery(%) |
|---|------------------------|------------------------------|--------|-------------|
| | | Proposed method ^a | ICP-MS | |
| Seawater samples 1 | 0 | 105 ± 2 | 107 | – |
| Seawater samples 2 | 0 | 110 ± 2 | 108 | – |
| Standard artificial seawater samples 1 ^b | 50 | 51 ± 1 | – | 102 |
| Standard artificial seawater samples 2 ^c | 50 | 51 ± 1 | – | 102 |

^a Each value is calculated from three experiments

^b The salinity of the standard artificial seawater sample 1 was 4.998

^c The salinity of the standard artificial seawater sample 2 was 29.998

which indicated that the GC/Au@MnO₂ lacked significant difference in the respect of current of stripping peak among the prepared electrodes. To check the repeatability, one modified electrode was repeatedly used for 24 times in 0.1 M acetate buffer (pH 5.0) containing 200 nM copper ions. In Fig. S7, the stripping peak current almost did not change and the RSD was 5.9%. In addition, the stability for one modified electrode was performed once a day for 15 days in 0.1 M acetate buffer (pH 5.0) containing 200 nM copper ions. The current had no obvious changes with only decreased 3.7% after 15 days. Hence, the modified electrode had good reproducibility and repeatability.

It is a challenging task to detect copper ions accurately in the real sample without interference. Thus, the interference study was evaluated by adding some probably interfering metals under the optimized working conditions in the solution with 100 nM copper ions. The 100-fold Ca²⁺, Zn²⁺, Mn²⁺, K⁺, Mg²⁺, Co²⁺ and anion NO₃⁻, SO₄²⁻, 50-fold Fe³⁺, Cd²⁺, 10-fold Bi³⁺, Pb²⁺, have no obvious interference in the determination of copper ions (<5% of response current change). These results strongly shows that the Au@MnO₂ modified electrode possess a great potential for online monitoring of copper ions in real seawater environment.

Analytical applications

To examine the practical application of the Au@MnO₂ electrode, the real seawater samples analysis had been performed. Furthermore, standard artificial seawater were also applied for the detection of copper ions. The salinity of the standard artificial seawater sample 1 was 4.998, and that of sample 2 was 29.998. Standard addition method was used for quantitative analysis. Recovery (%) was used to verify the accuracy of our method. A comparison of results in seawater between the paper method and ICP-MS were displayed in Table 2. The results indicates that the paper method is reliable and suitable for analysis of copper in seawater.

Conclusions

In summary, a novel and effective core-shell microsphere Au@MnO₂ modified electrode was successfully fabricated for sensitive determination of copper ions in real seawater sample and standard artificial seawater. The synthesis method was relatively uncomplicated and accessible compared to other reported methods. The tolerance of the Au@MnO₂ modified electrode to the pH value was poor, and the detection of the LOD was not particularly low. But this new modified electrode shows good repeatability and reproducibility. The Au@MnO₂ modified GCE facilitates to accurately detect copper ions in seawater. Accordingly, the fabricated electrode will be of great benefit to investigate the effects of copper ions in seawater.

Acknowledgements This work was financially supported by the National Natural Science Foundation of China (21575080), the Youth Innovation Promotion Association (2011170), and the Equipment Development Project (YZ201558) of Chinese Academy of Sciences.

Compliance with ethical standards The author(s) declare that they have no competing interests.

References

1. Fathi SA, Yafthian MR (2009) Enrichment of trace amounts of copper(II) ions in water samples using octadecyl silica disks modified by a Schiff base ionophore prior to flame atomic absorption spectrometric determination. *J Hazard Mater* 164:133–137
2. Zhang GS, Liu DY, Wu HF, Chen LL, Han QX (2012) Heavy metal contamination in the marine organisms in Yantai coast, northern Yellow Sea of China. *Ecotoxicology* 21:1726–1733
3. Stuart LB, Zirino A (1993) Behavior and calibration of the copper(II) ion-selective electrode in high chloride media and marine waters. *Anal Chem* 65:2583–2589
4. Zhang YF, Li R, Xue QW, Li HB, Liu JF (2015) Colorimetric determination of copper(II) using a polyamine-functionalized gold nanoparticle probe. *Microchim Acta* 182:1677–1683
5. Manzoori JL, Amjadi M, Darvishnejad M (2012) Separation and preconcentration of trace quantities of copper ion using modified alumina nanoparticles, and its determination by flame atomic absorption spectrometry. *Microchim Acta* 176:437–443
6. Wu JF, Boyle EA (1997) Low blank preconcentration technique for the determination of lead, copper, and cadmium in small-volume seawater samples by isotope dilution ICP-MS. *Anal Chem* 69:2464–2470
7. Zhang G, Liu D, Wu H, Chen L, Han Q (2012) Heavy metal contamination in the marine organisms in Yantai coast, northern Yellow Sea of China. *Ecotoxicology* 21:1726–1733
8. Vuković J, Matsuoka S, Yoshimura K, Grdinić V, Grubešić RJ, Županić O (2007) Simultaneous determination of traces of heavy metals by solid-phase spectrophotometry. *Talanta* 71:2085–2091
9. Hu J, Guo F, Wang L (2017) Voltammetric determination of nitrite by using a glassy carbon electrode modified with a self-assembled nanocomposite prepared from CdTe quantum dots, cetyltrimethylammonium bromide, chitosan and multiwalled carbon nanotubes. *Microchim Acta* 184:4637–4646
10. Yerga DM, Martos IA, Lopez MC, Henry CS, Abedul MT (2017) Point-of-need simultaneous electrochemical detection of lead and cadmium using low-cost stencil-printed transparency electrodes. *Anal Chim Acta* 981:24–33
11. Gao WY, Hui P, Qi LM, Liu ZY, Zhang W, Xu GB (2017) Determination of copper(II) based on its inhibitory effect on the cathodic electrochemiluminescence of lucigenin. *Microchim Acta* 184:693–697
12. Wang N, Dai HX, Wang DL, Ma HY, Lin M (2017) Determination of copper ions using a phytic acid/polypyrrole nanowires modified glassy carbon electrode. *Mater Sci Eng* 76:139–143
13. Lu ZW, Zhang JJ, Dai WL, Lin XN, Ye JP, Ye JS (2017) A screen-printed carbon electrode modified with a bismuth film and gold nanoparticles for simultaneous stripping voltammetric determination of Zn(II), Pb(II) and Cu(II). *Microchim Acta* 184:4731–4740
14. Liu M, Pan QW, Pan W, Zhu Y, Hu XP, Han HT, Wang CC, Shen DZ (2017) In-situ synthesis of reduced graphene oxide/gold nanoparticles modified electrode for speciation analysis of copper in seawater. *Talanta* 174:500–506
15. Gao C, Yu XY, Xiong SQ, Liu JH, Huang XJ (2013) Electrochemical detection of arsenic(III) completely free from noble metal: Fe₃O₄?

- microspheres-room temperature ionic liquid composite showing better performance than gold. *Anal Chem* 85:2673–2680
16. Han RP, Lu Z, Zou W, Tong WD, Shi J, Jun YJ (2006) Removal of copper(II) and lead(II) from aqueous solution by manganese oxide coated sand II Equilibrium study and competitive adsorption. *J Hazard Mater* 137:480–488
 17. Zhang G, Liu F, Liu H, Qu J, Liu R (2014) Respective role of Fe and Mn oxide contents for arsenic sorption in iron and manganese binary oxide: an X-ray absorption spectroscopy investigation. *Environ Sci Technol* 48:10316–10322
 18. Puppa LD, Komarek M, Bordas F, Bollinger JC, Joussein E (2013) Adsorption of copper, cadmium, lead and zinc onto a synthetic manganese oxide. *J Colloid Interface Sci* 399:99–106
 19. Qin Q, Wang Q, Fu D, Ma J (2011) An efficient approach for Pb(II) and Cd(II) removal using manganese dioxide formed in situ. *Chem Eng J* 172:68–74
 20. Zaman MI, Mustafa S, Khan S, Xing B (2009) Heavy metal desorption kinetic as affected by of anions complexation onto manganese dioxide surfaces. *Chemosphere* 77:747–755
 21. Veeramani V, Dinesh B, Chen SM (2016) Electrochemical synthesis of Au-MnO_2 on electrophoretically prepared graphene nanocomposite for high performance supercapacitor and biosensor applications. *J Mater Chem A* 4:3304–3315
 22. Qiu TF, Luo B, Michael G, Eser MA, Hao L, Wang XJ, Shi L, Jin MH, Zhi LJ (2014) Au@MnO_2 Core-Shell nanomesh electrodes for transparent flexible supercapacitors. *Small* 10:4136–4141
 23. Gnanaprakasam P, Jeena SE, Premnath D, Selvaraju T (2016) Simple and robust green synthesis of AuNPs on reduced graphene oxide for the simultaneous detection of toxic heavy metal ions and bioremediation using bacterium as the scavenger. *Electrochemistry* 28:1885–1893
 24. Prosper KY, Sean R, James D (2016) Gold nanoparticle modified screen-printed carbon arrays for the simultaneous electrochemical analysis of lead and copper in tap water. *Microchim Acta* 183:2361–2368
 25. Huang S, Lu SY, Huang CS, Sheng JR, Su W (2015) Sensitive and selective stripping voltammetric determination of copper(II) using a glassy carbon electrode modified with amino-reduced graphene oxide and β -cyclodextrin. *Microchim Acta* 182:2529–2539
 26. Megha AD, Raimonda C, Almira R, Mahendra DS, Arunas R (2018) EDTA_PANI/SWCNTs nanocomposite modified electrode for electrochemical determination of copper (II), lead (II) and mercury (II) ions. *Electrochim Acta* 259:930–938
 27. Ting SL, Ee SJ, Arundithi A, Kam CL, Peng C (2015) Graphene quantum dots functionalized gold nanoparticles for sensitive electrochemical detection of heavy metal ions. *Electrochim Acta* 172:7–11
 28. Clara PR, Julio BA, Nuria S, Jose MD, Cristina A, Joan DP, Miquel E (2017) Ag nanoparticles drop-casting modification of screen-printed electrodes for the simultaneous Voltammetric determination of Cu(II) and Pb(II). *Sensors* 17:1458–1469
 29. Geng S, Lin SM, Li NB, Luo HQ (2017) Polyethylene glycol capped ZnO quantum dots as a fluorescent probe for determining copper(II) ion. *Sensor Actuat B-Chem* 253:137–143
 30. Zheng X, Pan J, Gao L, Wei X, Dai J, Shi W, Yan Y (2015) Silica nanoparticles doped with a europium(III) complex and coated with an ion imprinted polymer for rapid determination of copper(II). *Microchim Acta* 182:753–761
 31. Paul RL, Cartwright A (1986) The mechanism of the deposition of manganese dioxide part II electrode impedance studies. *J Electroanal Chem* 201:113–122
 32. Andrew JG, Bernt J, Yaser B, Jessica A, Scott WD (2016) Dynamic electrodeposition of manganese dioxide: temporal variation in the electrodeposition mechanism. *J Electrochem Soc* 163:305–312